


INSTRUCTIONS FOR USE – PLEASE READ CAREFULLY

PRODUCT – EASIFLUSH STOPCOCK

This IFU is for the EasiFlush Range [Standalone & Line Mounted]

Instructions

1. Peel open package and remove set.
2. Ensure the stopcock is in the all ports open position, then prime the extension set according to the facility protocol, taking care to ensure the Needle-Free Site is fully primed and all air is expelled.
3. Use aseptic technique. To access port: Swab the valve port according to the facility protocol prior to each activation. We recommend swabbing with agents such as 70% IPA, Betadine or Chlorhexadine. We recommend swabbing for a minimum of 30 seconds and allow 30 seconds drying time for alcohol-based agents or 1 minute for aqueous based agents.
4. Rotate handle to control fluid flow.
5. Flow will be through ports aligned with arrow indicators on handle.
6. Use **'all ports open' position of the handle** in order to establish a continuous flow through the entire stopcock and the luer activated port. Continuous flow occurs from the patient distal port through the valve to the patient proximal port.
7. During IV applications use **'all ports open' position of the handle**, except for when side port is in use. Prior to detaching a syringe from the luer activated valve, handle position should be closed. Make sure syringe is depressurised in order to avoid fluid drop from syringe.
8. Flush the line according to hospital protocol

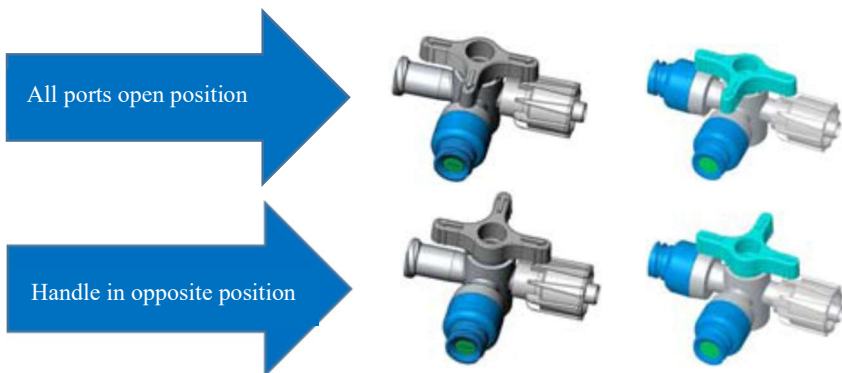

Special Instructions for blood sampling

1. Turn handle to 'Two ports open' position to allow sampling through the side needle free port.
2. Draw blood sample with a needle-free syringe through the luer-activated side port.
3. Prior to detaching a syringe from the luer activated valve, return handle to opposite position.
4. Flush the line according to hospital protocol.

See how it works



INSTRUCTIONS FOR USE – PLEASE READ CAREFULLY

PRODUCT – EASIFLUSH STOPCOCK

This IFU is for the EasiFlush Range [Standalone & Line Mounted]

The minimal residual volume luer-activated stopcock is indicated for fluid flow directional control and providing access port(s) for administration of solutions. Typical uses include intravenous fluid administration and transfusion.

CAUTIONS

- Store at room temperature
- Do not use if package is open or damaged.
- This device has a 5-year shelf life. Check expiry date on device packet before use
- For single use only. Do not re-sterilise.
- Handle package in a manner that will prevent accidental puncture.
- Do not clamp catheter or extension set while flushing or disconnecting the syringe or administration set from the Needle-Free Site.
- Maximum pressure 29 psi (2 bar)
- All ports are NOT necessarily closed when handle is turned 45° from ports.
- Verify appropriate handle position according to instruction below.



- Malfunctioning of the valve might occur if non-standard luer is used.
- Do not use needles to access valve port(s)
- The recommended duration of use for standalone devices is 96 hours
- The recommended duration of use for line mounted devices is 72 hours
- **The recommended duration of use for aggressive solutions is 24 hours for both line mounted and standalone devices**
- The maximum number of activations for line mounted and standalone devices is 96
- After use this product may be a potential biohazard. Dispose of device after use in accordance with applicable laws and regulations.

